

Descalvado sand for high-dose dosimetry

M.I. Teixeira^a, Gilberto M. Ferraz^{b,c}, Linda V.E. Caldas^{a,*}

^a*Instituto de Pesquisas Energéticas e Nucleares, Comissão Nacional de Energia Nuclear, Rua Prof. Lineu Prestes, 2242 São Paulo, Brazil*

^b*Instituto de Física, Universidade de São Paulo, Rua do Matão, s/n – São Paulo, Brazil*

^c*Faculdade Tecnologia e Ciências Exatas, Universidade São Judas Tadeu, Rua Taquari, 546 – São Paulo, Brazil*

Abstract

Brazilian beach sand has already shown usefulness for high-dose dosimetry using the electronic paramagnetic resonance (EPR) and thermoluminescence (TL) techniques. In this work sand samples from Descalvado were studied in relation to their main dosimetric properties. The EPR signal grows significantly in function of absorbed dose for g of 2.000 and 1.996. All studied sand samples can be used as EPR dosimeters for different applications in medical, agricultural and industrial areas.

© 2007 Elsevier Ltd. All rights reserved.

Keywords: Electronic paramagnetic resonance; Sand; Radiation dosimetry

1. Introduction

Sand samples were investigated with the purpose to verify the possibility of their use in dosimetric procedures of irradiation (high doses). Advances in irradiation technologies made possible commercial processes as sterilization, pasteurization, food preservation and treatment of various materials (McLaughlin et al., 1989; Farrar, 1999). Radiation processing at irradiation facilities requires a quality control program. The verification of absorbed doses is an essential procedure of such a control. Several kinds of dosimeters have been proposed, tested, and are presently in use for this purpose (McLaughlin et al., 1989). Propositions of dosimetric material easily found in the nature, as sand or commercial products as glass, were already studied (Vaijapurkar and Bhatnagar, 1993; Vaijapurkar et al., 1998; Quezada and Caldas, 1999; Caldas and Teixeira, 2002; Rodrigues and Caldas, 2002; Caldas et al., 2006).

The main component of sand is quartz (SiO_2), and its electronic paramagnetic resonance (EPR) properties received a great attention in literature; Griscom (1990) published a review paper of this important insulating material. Marfunin (1979) and Ikeya (1993) cited the main paramagnetic defects in quartz.

In this work sand samples from Descalvado, an inland city of São Paulo State, Brazil, were studied. Descalvado is the city that produces most of the sand used in the Brazilian glass industry. These sand samples contain high pureness and controlled concentrations of heavy minerals presenting steady physical and chemical characteristics, in compliance with the requirements in the area for the manufacture of glasses, silicates and ceramics. The industrial quartzous sand samples are produced by special equipment that confers steady physical characteristics to the end items, surpassing the very demanding specifications of the casting market. Their main dosimetric properties as response reproducibility, batch uniformity and calibration curves were investigated in order to trace a comparative study with the results of Brazilian beach sand (Teixeira and Caldas, 2004; Teixeira et al., 2005). The studied sand samples can be utilized as EPR dosimeters for different applications in medical, agricultural and industrial areas.

2. Materials and methods

Sand samples used in the present work proceed from a Descalvado natural reserve, São Paulo, Brazil. Two types of sand are manufactured there: one type for the glass industry and another type for the casting market, presented in different granulometries. These sand samples were called in this

* Corresponding author. Tel./fax: +55 11 3133 9716.
E-mail address: lcaldas@ipen.br (L.V.E. Caldas).

work as DSG (Descalvado sand for glass industry) and DSC (Descalvado sand for casting), respectively.

Sand was bolted, and grains were obtained between 0.180 and 0.075 mm diameter. The sand samples were washed with a chloridric acid solution 1 N (1 molar); after that, distilled water was used to remove the HCl and the organic impurities (Vaijapurkar and Bhatnagar, 1993). The wet sand samples were dried using an electric oven, Formitex, at 150 °C/50 min.

Magnetic particles (mainly iron) were removed from the sand samples using a magnetic separator (S.G. Frantz Com. Ind., Isodynamic, model L-1).

The samples were packed in aluminum foils and in black plastic bags for the irradiations, following the facility procedure. The irradiations were performed in air (room temperature) using a Gamma-Cell 220 system (^{60}Co , dose rate of 3.67 kGy/h) of the Center of Radiation Technology, IPEN. The irradiations were performed at ambient temperature, and the samples were fixed between 3 mm thick polymethyl methacrylate plates (Lucite), to guarantee the occurrence of electronic equilibrium during the irradiations.

Thermal treatments of 500 °C/1 h were applied to the glass samples for reutilization. The EPR measurements were carried out using a Bruker EMX spectrometer with a rectangular cavity (ER4102 ST), at room temperature, with microwave frequency of 9.76 GHz (X-band), microwave power of 0.202 mW, and with frequency and field modulation amplitude of 100 kHz and 0.1 mT, respectively. This EPR spectrometer belongs to the Multi-User Group of the Institute of Physics, University of São Paulo.

The sand samples were inserted in the equipment resonant cavity using a pure quartz tube with an average mass of (150 ± 1) mg. These samples present a thermal fading of their EPR spectra of about 8% after 24 h post-irradiation (Caldas et al., 2006). Due to this thermal fading, all measurements in this work were taken exactly 1 h after the irradiations.

3. Results and discussion

3.1. EPR spectra

Some dosimetric properties were studied in this work for the verification of the possibility of utilization of sand samples for high-dose dosimetry. The EPR spectra obtained of the DSG (for glass) and DSC (for casting) sand samples, irradiated with different absorbed doses of 0.1, 1 and 5 kGy are shown in Figs. 1 and 2, respectively.

The g factor was obtained using the EPR spectrum of Mn^{2+} from a standard $\text{MgO}:\text{Mn}$ sample. The third and fourth lines of the six lines associated with Mn^{2+} appear at $g = 2.033$ and 1.181, respectively (Ikeya, 1993). The EPR spectra of DSG and DSC samples are shown in Fig. 3, using the Mn^{2+} line as reference.

The EPR spectra of DSG and DSC samples present two g -factors at 2.000 and 1.996. These signals are formed in quartz grains present mainly in sand: 97–99%. These EPR signals were observed by Teixeira et al. (2005) in some Brazilian beach sand samples after irradiation. The signal at $g = 2.000$ corresponds

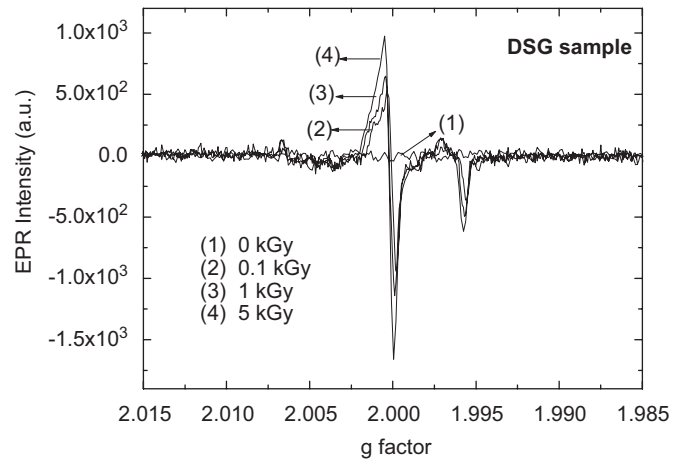


Fig. 1. EPR spectra of the DSG sand samples irradiated to different absorbed doses (^{60}Co).

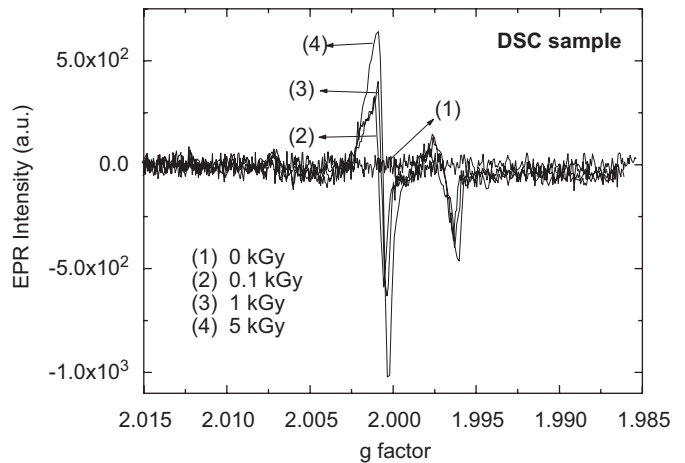


Fig. 2. EPR spectra of the DSC sand samples irradiated to different absorbed doses (^{60}Co).

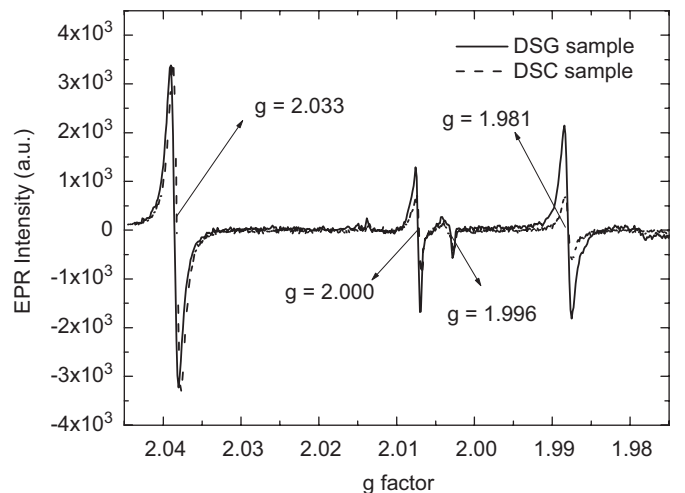


Fig. 3. EPR spectra of the DSG and DSC sand samples using Mn^{2+} as reference (^{60}Co , 5 kGy).

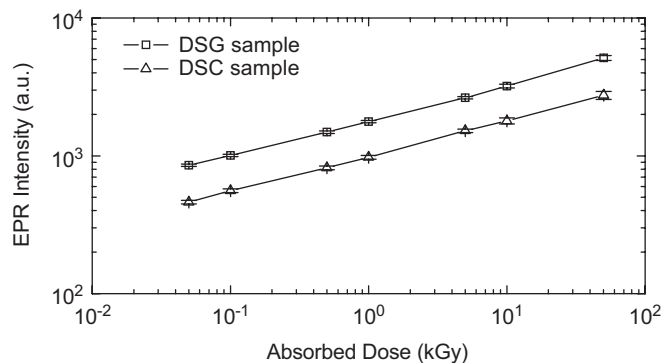


Fig. 4. Calibration curves of the EPR signal at $g = 2.000$ for DSG and DSC sand samples (^{60}Co).

to the counterfeit E'_1 center, according to Toyoda and Schwarcz (1997). The counterfeit E'_1 center is an electron trapped by an oxygen vacancy in the $[\text{SiO}_3]$ tetrahedron of quartz grains. However, this center is less stable than the original E'_1 center. The signal at $g = 1.996$ was not identified because it was less interesting from the dosimetric point of view.

3.2. Reproducibility

Groups of five sand samples (DSG and DSC) were submitted five times to the same procedure of thermal treatment at $500^\circ\text{C}/1\text{h}$ (defined for the reutilization), and irradiation (5 kGy), in order to study the response reproducibility. The maximum standard deviations obtained were approximately 4.1% for the DSG sand sample, and 4.9% for the DSC sand sample. The Ponta Negra Brazilian beach sand samples (Teixeira et al., 2005) presented 6.1% for the maximum standard deviation.

3.3. Dose response

The sand samples (DSG and DSC) were irradiated to various doses in the range between 50 Gy and 50 kGy. Fig. 4 presents the calibration curves for the materials. Sublinear behaviors were obtained in both cases. The maximum standard deviations obtained for these measurements were 2% and 3% of DSG and DSC sand samples, respectively.

In comparison with the dose response curve of Ponta Negra Brazilian beach sand samples (Teixeira et al., 2005), the DSG and DSC samples presented a greater region of sublinearity before the saturation. This region starts at 50 Gy and can be extended up to 50 kGy. Although the EPR spectra intensity of the Brazilian beach sand samples were more intense for high doses, these spectra present a clear saturation effect about 10 kGy.

4. Conclusions

The dose response curves obtained in this work show that the Descalvado sand samples may be applied to high-dose

dosimetry. The EPR signal grows significantly in function of the absorbed dose, for the g -factor at 2.000. Descalvado sand samples for glass industry present higher radiation sensitivity than that of the sand samples for casting. These samples present some advantages in relation to the Brazilian beach sand samples, as a better reproducibility and dose response curve in a greater dose interval up to 50 kGy.

The basic advantage of sand samples is their very low cost. Sand samples may be applied to dosimetry in the main radiation processes of seed stimulation, mutation breeding, industrial radiography, insect population control, pasteurization and water purification.

Acknowledgments

The authors thank Mr. Manoel J.B. Cordova, from Mineração Jundu Ltda., Descalvado, São Paulo, Brazil, for providing the sand samples, and to Conselho Nacional de Desenvolvimento Científico e Tecnológico (CNPq), and Fundação de Amparo à Pesquisa do Estado de São Paulo (FAPESP), Brazil, for partial financial support.

References

- Caldas, L.V.E., Teixeira, M.I., 2002. Commercial glass for high doses using different dosimetric techniques. *Radiat. Prot. Dosim.* 100 (1–4), 149–152.
- Caldas, L.V.E., Teixeira, M.I., Ferraz, G.M., 2006. Influence of thermal treatments on the response of sand radiation detectors for high-dose dosimetry. *Radiat. Prot. Dosim.* 120, 230–234.
- Farrar, H., 1999. Dosimetry standards for radiation processing. In: *Proceedings of Symposium Techniques for High Dose Dosimetry in Industry, Agriculture and Medicine*, Vienna, November 1998. AIEA-TEC DOC-1070, pp. 307–311.
- Griscom, D.L., 1990. Electron spin resonance investigations of defects and defects process in amorphous silicon dioxide. *Rev. Solid State Sci.* 4, 565–599.
- Ikeya, M., 1993. *New Applications of Electron Spin Resonance—Dating, Dosimetry and Microscopy*, first ed. World Scientific, Singapore.
- Marfunin, A.S., 1979. *Spectroscopy, Luminescence and Radiation Centers in Minerals*. Springer, Berlin. ISBN 3-540-09070-3.
- McLaughlin, W.L., Boyd, A.W., Chadwick, K.H., McDonald, J.C., Miller, A., 1989. *Dosimetry for Radiation Processing*. Taylor & Francis, London. ISBN 0-85066-740-2.
- Quezada, V.A.C., Caldas, L.V.E., 1999. Glass detectors for dose determination in a flower irradiation process. *Radiat. Prot. Dosim.* 85 (1–4), 473–475.
- Rodrigues Jr., A.A., Caldas, L.V.E., 2002. Commercial plate window glass tested as routine dosimeter at a gamma irradiation facility. *Radiat. Phys. Chem.* 63, 765–767.
- Teixeira, M.I., Caldas, L.V.E., 2004. Sintered sand pellets for high-dose dosimetry. *Nucl. Instrum. Methods Phys. Res. B* 218, 194–197.
- Teixeira, M.I., Ferraz, G.M., Caldas, L.V.E., 2005. Sand for high-dose dosimetry using the EPR technique. *Appl. Radiat. Isot.* 62, 359–363.
- Toyoda, S., Schwarcz, H.P., 1997. Counterfeit E'_1 signal in quartz. *Radiat. Meas.* 27 (1), 59–66.
- Vaijapurkar, S.G., Bhatnagar, P.K., 1993. Low cost thermoluminescence (TL) gamma dosimeter for radiotherapy. *Nucl. Tracks Radiat. Meas.* 21 (2), 267–269.
- Vaijapurkar, S.G., Raman, R., Bhatnagar, P.K., 1998. Sand—a high gamma dose thermoluminescence dosimeter. *Radiat. Meas.* 29 (2), 223–226.